

SprintRay SportsGuard

Instructions for Use

Indications for Use

SprintRay SportsGuard resin is a light-curable, polymerizable material intended for the fabrication of appliances that cover the teeth and adjacent oral tissues to help prevent or reduce trauma to teeth, gingiva, lips, and jaws during athletic or recreational activities. This material is not cleared or classified for use in the manufacture of regulated medical devices.

Contraindications

SprintRay SportsGuard is contraindicated when:

- A patient is known to be allergic to any of the ingredients
- There is direct intraoral contact with resin that is not fully cured
- It is used for any purpose other than its indications for use.

Appliance Description

SprintRay SportsGuard is a photopolymer (meth)acrylate resin material used in conjunction with a 3D printer and a scanned 3D image in a dental office to build appliances that are worn over the top row of teeth during sports to help prevent an oral injury. Sports Guard is an alternative to traditional materials for the fabrication of Sports Guards. SprintRay Sports Guard resin is offered in clear, red, and blue shades. It is intended exclusively for professional dental work.

Printing and Hardware Parameters

The appliance specifications have been only validated using the following hardware and software. Any products or processes not specified in this document have not been validated to meet the intended performance. Always refer to the SprintRay equipment user instructions for device setup, maintenance, and lifespan. Always refer to the SprintRay material Instruction for Use (IFU) for recommended design limits and proper validated equipment parameters.

SprintRay SportsGuard is intended exclusively for use by trained dental professionals.


- a. CAD File:** CAD file of treatment appliance in STL file format:
 - i. Upload an STL or SPR file to Cloud Dashboard Print Setup.
- b. Printer:** SprintRay Pro 2 3D printer
 - i. Pro 2: 35-micron XY resolution and energy of 25 mW/cm²

c. Software: Cloud Dashboard Print Setup

- i. STL file import
- ii. Manual/automatic orientation (preferred)

d. Printing Parameters

- i. Pro S and Pro 2: Automatically oriented on RayWare Cloud

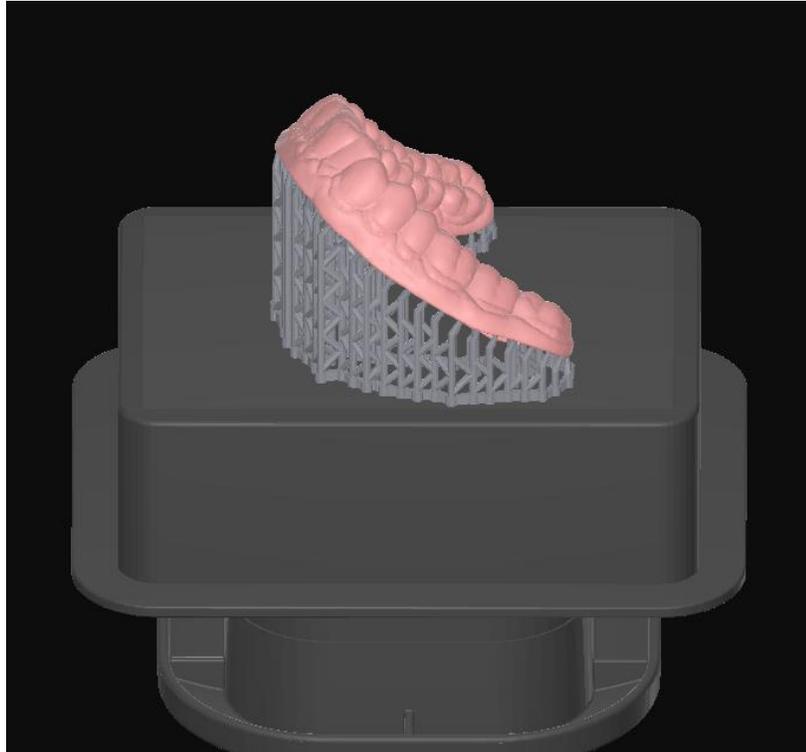

- ii. 100-micron layer thickness
- iii. Default support structures

e. Wash Device: SprintRay ProWash S or SprintRay Pro Wash/Dry

- i. 91% or higher IPA
- ii. Custom Multicycle: 3-minute wash chamber 1, 5-minute rinse chamber 2, 3-minute dry

f. Cure Device:

- i. SprintRay NanoCure
Use SprintRay-recommended curing times that are built in the device

Warning and Precautions

SprintRay SportsGuard appliances are non-toxic in fully post cured form and are classified as a biocompatible material. In uncured form, SportsGuard resin is classified as hazardous. When washing with solvent or grinding/polishing the appliance, do so in a well-ventilated area with

proper personal protective equipment including protective gloves, clothing, eyewear, and face protection when handling.

- **Skin Contact:** May cause skin irritation. If unprocessed resin contacts skin, wash thoroughly with soap and water. May cause an allergic skin reaction. If skin sensitization occurs, stop using. If dermatitis or other symptoms persist, seek medical assistance.
- **Inhalation:** High vapor concentration may cause headache, irritation of eyes and/or respiratory system. If exposed to a high concentration of vapor or mist, move to fresh air. Use oxygen or artificial respiration as required.
- **Eye Contact:** Wash the contacted area thoroughly with water.
- **Ingestion:** Contact your regional poison control center immediately.
- **Use of Incompatible Components:** Do not substitute any of the components of the device system, i.e., appliance photopolymer materials, bonding systems, scanners, 3D printers, post-curing units, CAD/CAM software, templates, and tools. Use only those specifically identified in this labeling. Unauthorized changes may result in a appliance that is outside of specification. Contact the manufacturer for compatible components.
- Maintain and calibrate equipment according to manufacturer instructions.
- **Minor Color Differences:** Shade variance may occur due to inadequate shaking and mixing of the original packaging before use; inadequate stirring in the resin tank before use; insufficient post-curing.

Storage

- **Material Reuse:** The remaining resin in the resin tank can be reused. You may use a filter to ensure the resin is free from any cured particles to avoid print failures. The remaining material in the tank can be poured back into the resin bottle upon filtration. This process can be repeated until the material in the bottle is fully consumed. Please note that in the case of reuse, the resin must be filtered and poured back into the same bottle.
- Store SprintRay SportsGuard resin at 15-25°C (60-77°F) and avoid direct sunlight
- Keep the bottle closed and/or the tank lid securely attached when not in use
- Do not use SprintRay SportsGuard resin after the expiration date printed on the bottle
- Resin must be protected from exposure to light, as spontaneous polymerization is possible. The bottle must be tightly closed after every usage.



Do not use expired resin as biocompatibility, performance, and print stability may be compromised.

Fabrication of Appliance

This resin was validated using the following workflow. Failure to follow the recommended practices may lead to undesired safety and performance implications. Any deviation from these instructions for use may negatively affect the physical and/or chemical qualities of the resin and the biocompatibility of the product.

Where applicable, refer to the Workflow Guide for detailed best practices for producing specific appliance types with SprintRay resins.

Designing

The appliance is designed in STL file format by a dental design service preferable SprintRay Cloud Design, or dental CAD software using digital anatomical data from the patient. Refer to Appliance Design Guide <https://support.sprinray.com/s/article/Appliance-Design-Guidelines> for recommended design limits. This STL file is delivered to the clinician for fabrication.

3D Printing

For the validated devices' (including 3D printers and post-processing units) set-up, usage, on-site validation, Maintenance, and Troubleshooting, refer to the original equipment manufacturer (OEM) labeling for these compatible system components. It can be found online at:

- Printing devices: <https://support.sprinray.com/s/printer>
- Post Curing Devices: <https://support.sprinray.com/s/cure>

Nesting on Cloud Dashboard Print Setup (Pro 2): Sign in to RayWare Cloud and select the appliance type; the algorithm will automatically orient and add supports. Select this material and use the desired layer thickness. Queue the job to your printer.

Printing on Pro 2: Ensure the Print Platform is clean, dry, securely placed, and locked on the platform-arm. Shake the resin bottle thoroughly for one minute, then pour into the resin tank up to at least the min fill line. From the printer touchscreen, assign the resin tank to the proper material and navigate to the printer queue. Start the print job.

Part and Support Removal

After your appliance has been printed, remove it from the print platform using a print removal Tool. Remove all supports using a flush cutter or round diamond disc. Cut as close as possible to the appliance to minimize the smoothing and finishing procedure.

Washing and Drying

Use $\geq 91\%$ IPA to wash the appliance using one of the following methods:

- SprintRay ProWash S and Pro Wash/Dry

- o Custom Multi-Cycle Wash – Wash/Rinse/Dry (3-min wash chamber 1, 5-min rinse chamber 2, 3-min dry)

Post Curing

Use the following post-curing equipment and processes. For SprintRay devices, use the recommended settings

- NanoCure (preprogrammed material profile)

Dry the part completely before post curing.

Finishing

You may remove the supports before or after washing the printed appliance. Use a flush cutter, or a diamond disk to remove all the supports. Try to cut as close as possible to the appliance to minimize the smoothing and polishing procedure.



Ensure the appliance is completely dry of Isopropyl Alcohol before post curing. It is advisable to use an air dryer or leave the appliance away from the light at an ambient temperature for a short time.

Polishing

Use a carbide burr to remove any stumps from supports. After, smooth any rough areas with a Scotch-Brite™/Fuzzies™ rotary hand tool piece. Lastly, apply a thin coat of mineral oil to the supported surface and use a cotton buffing rotary hand tool piece to remove debris from finishing and improve the sheen of the support nubs (optional). Wash and clean the appliance with a brush using soap and warm water.

Clean & Disinfect

Use a laboratory steamer to clean the appliance of all debris. After, use dish soap and a brush with warm water to further clean the appliance.


Disposal Considerations

Always follow federal, state, and local regulations for hazardous waste disposal. To ensure proper classification, consult your local regulations. US guidelines can be found in 40 CFR part 261.3. Liquid resin must be cured completely before regular disposal. Simply pour it into a clear container and expose it to direct sunlight until hardened or in one of the post cure boxes. SprintRay SportsGuard is not an environmental hazard in its final, fully cured state. Once cured,

it can be thrown away with regular trash.

Symbol Guide

The table below provides reference for symbols that may appear on the resin product label.

	Keep away from sunlight		Use-by date
	Consult instructions for use		European conformity
	Lot number		SKU number
	Manufacturer		Temperature limit
	UK Conformity Assessed (UKCA) Marking		Irritation
	Unique device identifier		Importer
	Indicates the authorized representative in Switzerland		Authorized representative in the European community
	Manufacturing date		Wear gloves
	UK responsible person		UK Conformity Assessed (UKCA) Marking

Additional Help & Support

We are here to support you throughout the implementation period of your new technology. Our experienced support technicians are available M - F from 6 AM - 5 PM PT at 800-914-8004.



IFU-XXX - Instructions For Use – SportsGuard
DCO#: 1950
Revision#: 1
Effective Date: 03/13/2026

Contact Information

For product assistance, please review help information at: <https://sprintray.com/digital-dentistry/>

To report product issues, please contact SprintRay at:
<https://support.sprintray.com/s/contactsupport>

Phone: 1-800-914-8004



Manufacturer information

SprintRay Inc.
2710 Media Center Dr., Suite #100A
Los Angeles, CA 90065, USA